

UNCLASSIFIED

AD NUMBER	
AD013879	
CLASSIFICATION CHANGES	
TO:	unclassified
FROM:	restricted
LIMITATION CHANGES	
TO: Approved for public release; distribution is unlimited.	
FROM: Distribution authorized to U.S. Gov't. agencies only; Administrative/Operational Use; 24 DEC 1952. Other requests shall be referred to Navy Department, Bureau of Ships, Washington, DC.	
AUTHORITY	
E.O. 10501 dtd 5 Nov 1953.	

THIS PAGE IS UNCLASSIFIED

RESTRICTED

AD No 13879
ASTIA FILE COPY

Report Number _____ Date 24 Sept. 1952 to 24 Dec. 1952

Subject INTERIM RESEARCH REPORT

FOR

RADIOPHOTOLUMINESCENT AND TENEBRESCENT GLASSES

NAVY DEPARTMENT BUREAU OF SHIPS ELECTRONICS DIVISIONS

NObsr-57016 NE-051551 2.3

By N . J. Kreidl

Chemical Research Director

Bausch & Lomb Optical Co.

Rochester 2, New York

RESTRICTED

BAUSCH & LOMB OPTICAL CO.

ROCHESTER 2, NEW YORK



June 24, 1953

Office of the Chief Signal Officer
Engineering and Technical Division
Washington 25, D. C.

Att: SIGGG-P

Subject: Contract N0bsr-57016
Interim Research Report

Gentlemen:

Enclosed are your copies of the following
Interim Research Report in connection with the sub-
ject contract:

Interim Research Report
Contract N0bsr-57016
for the period 24 September
to 24 December 1952

Very truly yours,

BAUSCH & LOMB OPTICAL CO.

C Woodward
Defense Contract Department

CTWolfard/sm
Encs.

AW 6/29/53



RESTRICTED

RESTRICTED

INTERIM RESEARCH REPORT

FOR

RADIOPHOTOLUMINESCENT AND TENEBRESCENT GLASSES

This report covers the period 24 September 1952 to 24 December 1952.

BAUSCH AND LOMB OPTICAL CO.

ROCHESTER 2, NEW YORK

NAVY DEPARTMENT BUREAU OF SHIPS ELECTRONICS DIVISIONS

NObsr-57016 NE-051551 2.3

WARNING: This document contains information affecting the national defense of the United States within the meaning of the Espionage Laws, Title 18, U.S.C., Sections 793 and 794. The transmission or the revelation of its contents in any manner to an unauthorized person is prohibited by law. Reproduction of this document in any form by other than activities of the Department of Defense and the Atomic Energy Commission is not authorized unless specifically approved by the Secretary of the Navy or the Chief of Naval Operations."

Copy No.

17

RESTRICTED

RESTRICTED

CONTENTS

	Page
Distribution List	1 - 3
Part I <u>Present Status</u>	
1.1 Purpose	4
1.2 General Factual Data	5
1.3 Detail Factual Data	7
Table I - Dosimeter Sensitivity and Predose as a Function of Batch Variation	8
Table II - Attempts to Improve the Durability of the Manganese Standard Glass	10
Part II <u>Program for Next Interval</u>	13
Project Performance and Schedule	14
Figure 1 - Sensitivity of a Direct Reading Dosimeter Glass by Colorimetry	15
Figure 2 - Sensitivity of a Direct Reading Dosimeter Glass by Spectrophotometry	16
Figure 3 - Sensitivity of a Direct Reading Dosimeter Glass by Density Difference Calculated from Spectrophotometric Curves (Fig. 2)	17
Fiscal Status - Contract NObsr-57016 (Inserted in certain copies only)	18

RESTRICTED

RESTRICTED

Distribution List

Copy No. 1	Office of the Chief of Naval Operations (Op-36) Department of the Navy Washington 25, D.C.
Copy No. 2	Chief, Bureau of Aeronautics (Code AE-54) Department of the Navy Washington 25, D.C.
Copy No. 3	Chief, Bureau of Medicine and Surgery (Atomic Defense Division) Department of the Navy Washington 25, D.C.
Copy No. 4	Office of Naval Research (Nuclear Physics Section) Department of the Navy Washington 25, D.C.
Copy No. 5	Commanding Officer Naval Medical Research Institute (Maynard Eicher) Building 17, Bethesda, Maryland
Copy No. 6	Commanding Officer (Code 996) U.S. Naval Radiological Defense Laboratory San Francisco 24, California
Copies No. 7 - 8	Commanding Officer U.S. Naval Radiological Defense Laboratory Nucleonics Division (Dr. Guthrie) San Francisco 24, California
Copy No. 9	Commanding Officer and Director U.S. Navy Electronics Laboratory San Diego 52, California
Copy No. 10	Commander, New York Naval Shipyard (Material Laboratory) Naval Base Brooklyn 1, New York
Copy No. 11	Director, Naval Research Laboratory Technical Information Division Washington 20, D.C.

RESTRICTED

RESTRICTED

Copy No. 12	Director, Naval Research Laboratory (Mr. Egli, Metallurgy Division) Washington 20, D.C.	
Copy No. 13	Director, Evans Signal Laboratory (Technical Reports Section) Belmar, New Jersey	
Copy No. 14	Director, Evans Signal Laboratory (Nucleonics Section, General) Engineering Branch Belmar, New Jersey	
Copy No. 15	Commanding General Air Research and Development Command P.O. Box 1395 Baltimore 3, Maryland Attention: Capt. S. Shwiller, RDRN	
Copy No. 16*	Department of the Air Force, Headquarters United States Air Force Washington 25, D. C. Attention: AFDRD-EQ-1	
Copy No. 17	Office of the Chief Signal Officer Engineering and Technical Division Washington 25, D.C. Attention: SIGGG-P	
Copy No. 18	Chairman, Radiation Instruments Branch (Technical Coordination Section) U.S. Atomic Energy Commission Division of Biology and Medicine Washington 25, D. C.	
Copies No. 19-28	Secretary, Panel on Radiological Instruments Armed Forces Special Weapons Project Post Office Box 2610 Washington 25, D. C.	
Copy No. 29	The President Army Field Forces Board No. 1 Fort Bragg, North Carolina	
Copies No. 30-33	Navy Department Bureau of Ships, Chief Attention: Code 327 Washington 25, D. C.	via: Naval Inspector of Ordnance c/o Bausch and Lomb Opt.Co. Rochester, New York

RESTRICTED

RESTRICTED

Copy No. 34	Naval Inspector of Ordnance c/o Bausch and Lomb Optical Co. Rochester 2, New York	
Copies No. 35-40	Navy Department Bureau of Ships, Chief via: Attention: Code 327 Washington 25, D. C.	Naval Inspector of Ordnance c/o Bausch & Lomb Opt. Co. Rochester, New York
Copy No. 41	Dr. W. A. Weyl School of Mineral Industries Pennsylvania State College State College, Pennsylvania	
Copy No. 42	Dr. G. Monk Senior Physicist Remote Control Engineering Div. Argonne National Laboratories P.O. Box 5207 Chicago 80, Illinois	
Copy No. 43	V. Young	
Copy No. 44	M. Scott	
Copy No. 45**	N. Kreidl	
Copy No. 46	H. Coleman	Copies 43-49 are Bausch and Lomb Copies
Copy No. 47	C. Cala	
Copy No. 48	A. Anderson	
Copy No. 49	T. Pett	

*Copy No. 16 exists only for summary or final reports.

**Copy No. 45 is circulated to Mr. C. Bausch and Mr. K. Reynolds.

RESTRICTED

RESTRICTED

1.

PART I

PRESENT STATUS

1.1 PURPOSE

The purpose of this investigation is to determine, in glasses, the causes of optical changes produced by X- or gamma radiation, to select and develop compositions which combine optimum indication and integration of X- or gamma radiation with desirable technological properties affecting their eventual manufacture, and to evaluate glasses which without radiation by X- or gamma rays will fluoresce in a manner similar to the existing dosimeter glass.

RESTRICTED

RESTRICTED

1.2 GENERAL FACTUAL DATA

1.2.1 Personnel

Hours Spent by Personnel on this Project			
Month Ending	<u>24 Oct.</u>	<u>23 Nov.</u>	<u>27 Dec.</u>
N. J. Kreidl Director of Research	31	36	-
T.G. Pett Head, Glass Physics Section	15	5	15
G. Blair Chemist	160	160	160
W. Kirchgessner Spectroscopist	32	9-1/2	21
J. Mogenhan Chemist	8	8	9
W. VandeMark Technician	13	8	-
G. Biel Technician	-	20	12
E. Herko Chemist	-	2	-
E. Simms Technician	-	1	-

1.2.2 Test Equipment

CP-95 (XN-3)/PD Radiac Computer Indicator, Serial No. 19 together with calibration standards supplied by the Polaroid Corporation, was used to obtain all readings on the radiophotoluminescent glass. Readings are given in N.U. (New Units). This unit was established by Dr. J. Schulman to relate a gamma radiation dose of 100r with a 100 unit reading with this instrument on a glass of specified sensitivity. In other words under proper conditions, N.U. readings will indicate the dosage in roentgens.

RESTRICTED

RESTRICTED

1.2.2 Test Equipment (Continued)

A Co⁶⁰ source was used for all exposures. This equipment was described in Interim Report 24 Feb. to 24 March 1952.

A Hunter Color-Color Difference Meter was used in evaluating color changes. This instrument is essentially a photometer measuring three factors - transmittance and 2 chromaticity factors. (Reference: R. S. Hunter, "Photoelectric Color-Color Difference Meter", J. Opt. Soc. Am., 38, (7), 661 (1948).

A Hardy Recording Spectrophotometer was used in evaluating changes of absorption in the visible range of the spectrum.

RESTRICTED

RESTRICTED

1.3 DETAIL FACTUAL DATA

1.3.1 Topic 1 - Present Radiophotoluminescent Glass

1.3.1.1 Sensitivity and Predose

1.3.1.1.1 Purpose

To classify available raw materials in relation to the present specifications on predose and sensitivity of the radiophotoluminescent glass specified for use in Radiac Detector DT-60/PD, Specification - MIL-D-16153C (Ships).

1.3.1.1.2 Experimental

As the result of discussions and correspondence with the Victor Chemical Works, it was suspected that iron might have been introduced into the rather abrasive aluminum metaphosphate from the iron equipment used in the milling operation. New raw materials supplied by Victor were used in making melts and the glasses were tested.

1.3.1.1.3 Results and Conclusions (Table I)

The results, as seen in Table I in comparing melts 1A4089 and 1A4105, verified our suspicions. The sensitivity of the glass increased from 43 to 128 N.U. when unmilled was substituted for milled material. Unmilled aluminum metaphosphate did not blend well with other batch materials, but satisfactory results were also achieved with aluminum metaphosphate that was milled in non-metallic equipment (Lot #E-9318), (Melt #1A4476). Crushed aluminum metaphosphate (Lot #E-8838), (Melt #1A4297) was found to be inferior.

RESTRICTED

RESTRICTED

TABLE I

Dosimeter Sensitivity and Predose as a Function of Batch Variation

<u>Melt No.</u>	<u>Batch</u>		<u>Remarks</u>
1A4089	$\text{Al}(\text{PO}_3)_3$	Victor - Lot #E-8768 (50%) (Milled in iron equipment)	<u>Readings:</u> <u>N.U.</u>
	$\text{Ba}(\text{PO}_3)_2$	Monsanto - Lot #20607 (25%)	
	KPO_3	Monsanto - Lot #2 (20%)	Predose 23
	KNO_3	Plant Material (5%)	Sensitivity 43
	AgPO_3	Monsanto - Lot #70293 (8%)	
<hr/>			
1A4105	Same as 1A4089 except with the substitution of:		<u>N.U.</u>
	$\text{Al}(\text{PO}_3)_3$	Victor - Lot #E-8760 (50%) (Unmilled)	Predose 24 Sensitivity 128
<hr/>			
1A4297	$\text{Al}(\text{PO}_3)_3$	Victor - Lot #E-8838 (50%) (Crushed)	<u>N.U.</u>
	$\text{Ba}(\text{PO}_3)_2$	Monsanto - Lot #50020 (25%)	
	KPO_3	Victor - Lot #E-9082 (20%)	Predose 44
	KNO_3	Plant Material (5%)	Sensitivity 81
	AgPO_3	Monsanto - Lot #70293 (8%)	
<hr/>			
1A4476	Same as 1A4297 except with the substitution of:		<u>N.U.</u>
	$\text{Al}(\text{PO}_3)_3$	Victor - Lot #E-9318 (50%) (Milled in non-metallic equipment)	Predose 36 Sensitivity 114

RESTRICTED

RESTRICTED

1.3.2 Topic 2 - Standard Glass

1.3.2.1 Purpose

At the request of Mr. Rainey, Bureau of Ships, work was again resumed on this phase of the program to investigate glasses that might have an intensity of fluorescence similar to a silver phosphate glass dosed to 150r in respect to performance and possible improvements of durability.

1.3.2.2 Experimental

Experiments on performance of the present E-9272 type were started. Two experimental melts were made, that were slight revisions of a composition (Melt No. 1A4133) previously tried for the Polaroid Corporation, that had given very satisfactory performance, in the hope of improving its durability (see letter of 24 June 1952 to Chief, Bureau of Ships, Code 854, from Dr. W. A. Shurcliff).

1.3.2.3 Results and Conclusions (Table II)

Results on the performance of the present E-9272 will be discussed in the next report as the work is still in progress.

Results on durability improvements were considered unpromising as the chemical changes considered necessary adversely affected fluorescence performance and further work was discontinued in agreement with the Bureau of Ships.

RESTRICTED

RESTRICTED

TABLE II

Attempts to Improve the Durability of the
Manganese Standard Glass

<u>Composition - Wt. %</u>		
<u>Oxide</u>	<u>Melt No. 1A4395</u>	<u>Melt No. 1A4497</u>
SiO ₂	41.5	37.41
Na ₂ O	23.0	26.06
B ₂ O ₃	32.5	36.51
MnO ₂	0.01	0.01
As ₂ O ₃	0.0005	0.0005
Sb ₂ O ₃	0.0005	0.0005
MgO		1.0
CaO		2.0
ZrO ₂		1.0
Al ₂ O ₃	3.0	2.0
Color of Fluorescent Light	Yellow	Orange
Intensity	Approx. 150 N.U.	Approx. 150 N.U.
Durability	No Improvement	No Improvement

* This is composition of Melt No. 1A4133, see text.

** Added in excess of 100% to this base.

RESTRICTED

RESTRICTED

1.3.3 Topic 3 - Tenebrescent Glass

1.3.3.1 Purpose

Investigation of causes of changes in absorption under irradiation, especially if useful in the development of glasses for direct reading dosimeters ("tenebrescent glasses").

1.3.3.2 Experimental

An experimental remelt (1A4248) was made in a 4" zircon crucible and 2 blocks of glass were cast of the most promising composition previously reported, viz.:

$\text{Al}(\text{PO}_3)_3$ - 50 wt.%

$\text{Ba}(\text{FO}_3)_2$ - 25 wt.%

KPO_3 - 20 wt.%

KNO_3 - 5 wt.%

AgPO_3 - .8 wt.%

BaF_2 - 1 wt.%

} Added in excess of 100%

The blocks were finished in the following manner:

Dimensions - 39 x 48.5 x 57mm thick.

Finish - The 2 (39 x 48.5) surfaces were polished.

The other 4 surfaces were ground to #80 grit finish and painted with black paint.

Readings were taken of the absorption bands formed in the visible spectrum after exposures of 20, 40, 80, 160, 320, 640r on a Hardy Recording Spectrophotometer and a Hunter

RESTRICTED

RESTRICTED

Color-Color Difference Meter (see Figs. 1, 2, 3).

1.3.3.3 Results and Conclusions

Both the Hardy and Hunter instruments give measurable and linear readings starting at 20r exposure as can be seen from Figs. 1, 2, 3. A visible change was detected on the exposed sample at the 80r level. A control sample was used on all readings. All these findings are rather unique at the present stage of knowledge. Possibly the color change could be enhanced by using greater thickness and by the use of an integrating device such as coating a long cylinder with white paint and enclosing this assembly in an opaque container so that only one surface would be exposed, as suggested by Dr. J. Schulman of the Naval Research Laboratory. Also, the strong absorption band formed by irradiation in the near U.V. may permit the use of the emission change in a fluorescent material to obtain a more sensitive response.

The direct coloration of glass may be useful in a direct reading dosimeter if greater sensitivity can be obtained. However, this glass is not now considered practical, as an untrained observer will not easily recognize a change much below 200r in a piece of the largest practical dimensions, since it happens to occur in a part of the spectrum to which the human eye is most insensitive.

RESTRICTED

RESTRICTED

2.

PART II

PROGRAM FOR NEXT INTERVAL

2.1 In agreement with Mr. Rainey, Bureau of Ships, the remaining time on this contract will be utilized to complete work on three phases, namely:

- a) The investigation of the effect of heat treatment to erase previous exposure history in the radiophotoluminescent dosimeter glass and to evaluate second exposure sensitivity after this erasing.
- b) The investigation of reproducibility of the manganese standard glass (E-9272 type) in production melting.
- c) Whatever may be found necessary to complete the contract adequately.

RESTRICTED

RESTRICTED


BAUSCH AND LOMB OPTICAL CO.

Project Performance and Schedule
Index No. NE-051551

Contract NObsr-57016

Report Date 24 December 1952

Period Covered 24 September 1952 to December 1952

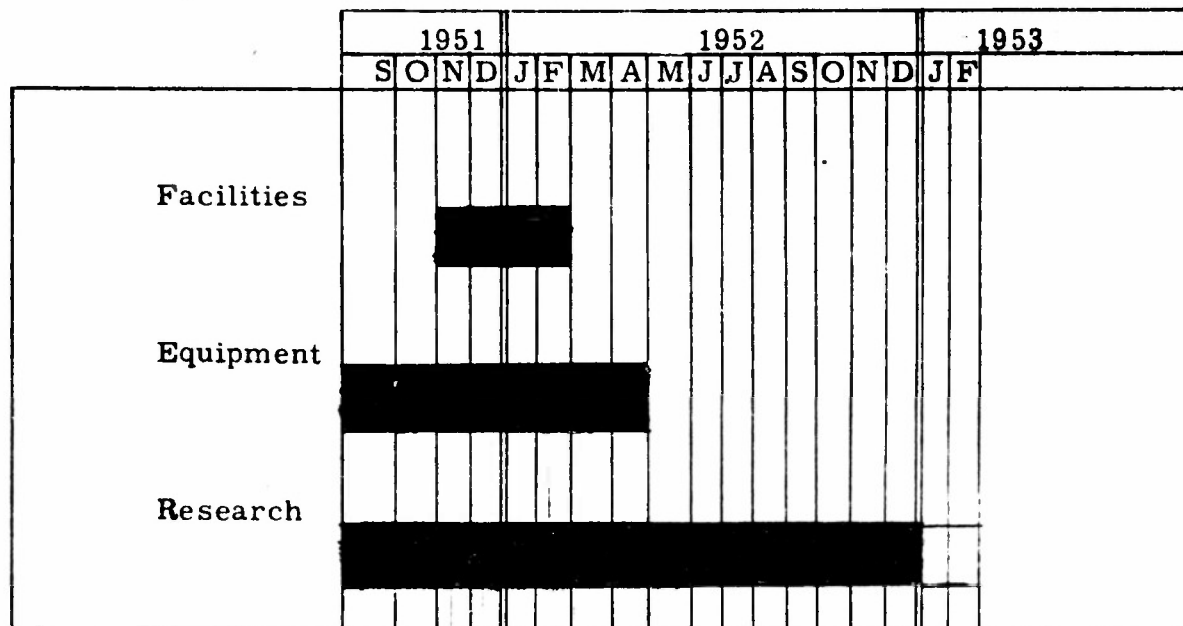

Projected Work



Completed Work

RESTRICTED

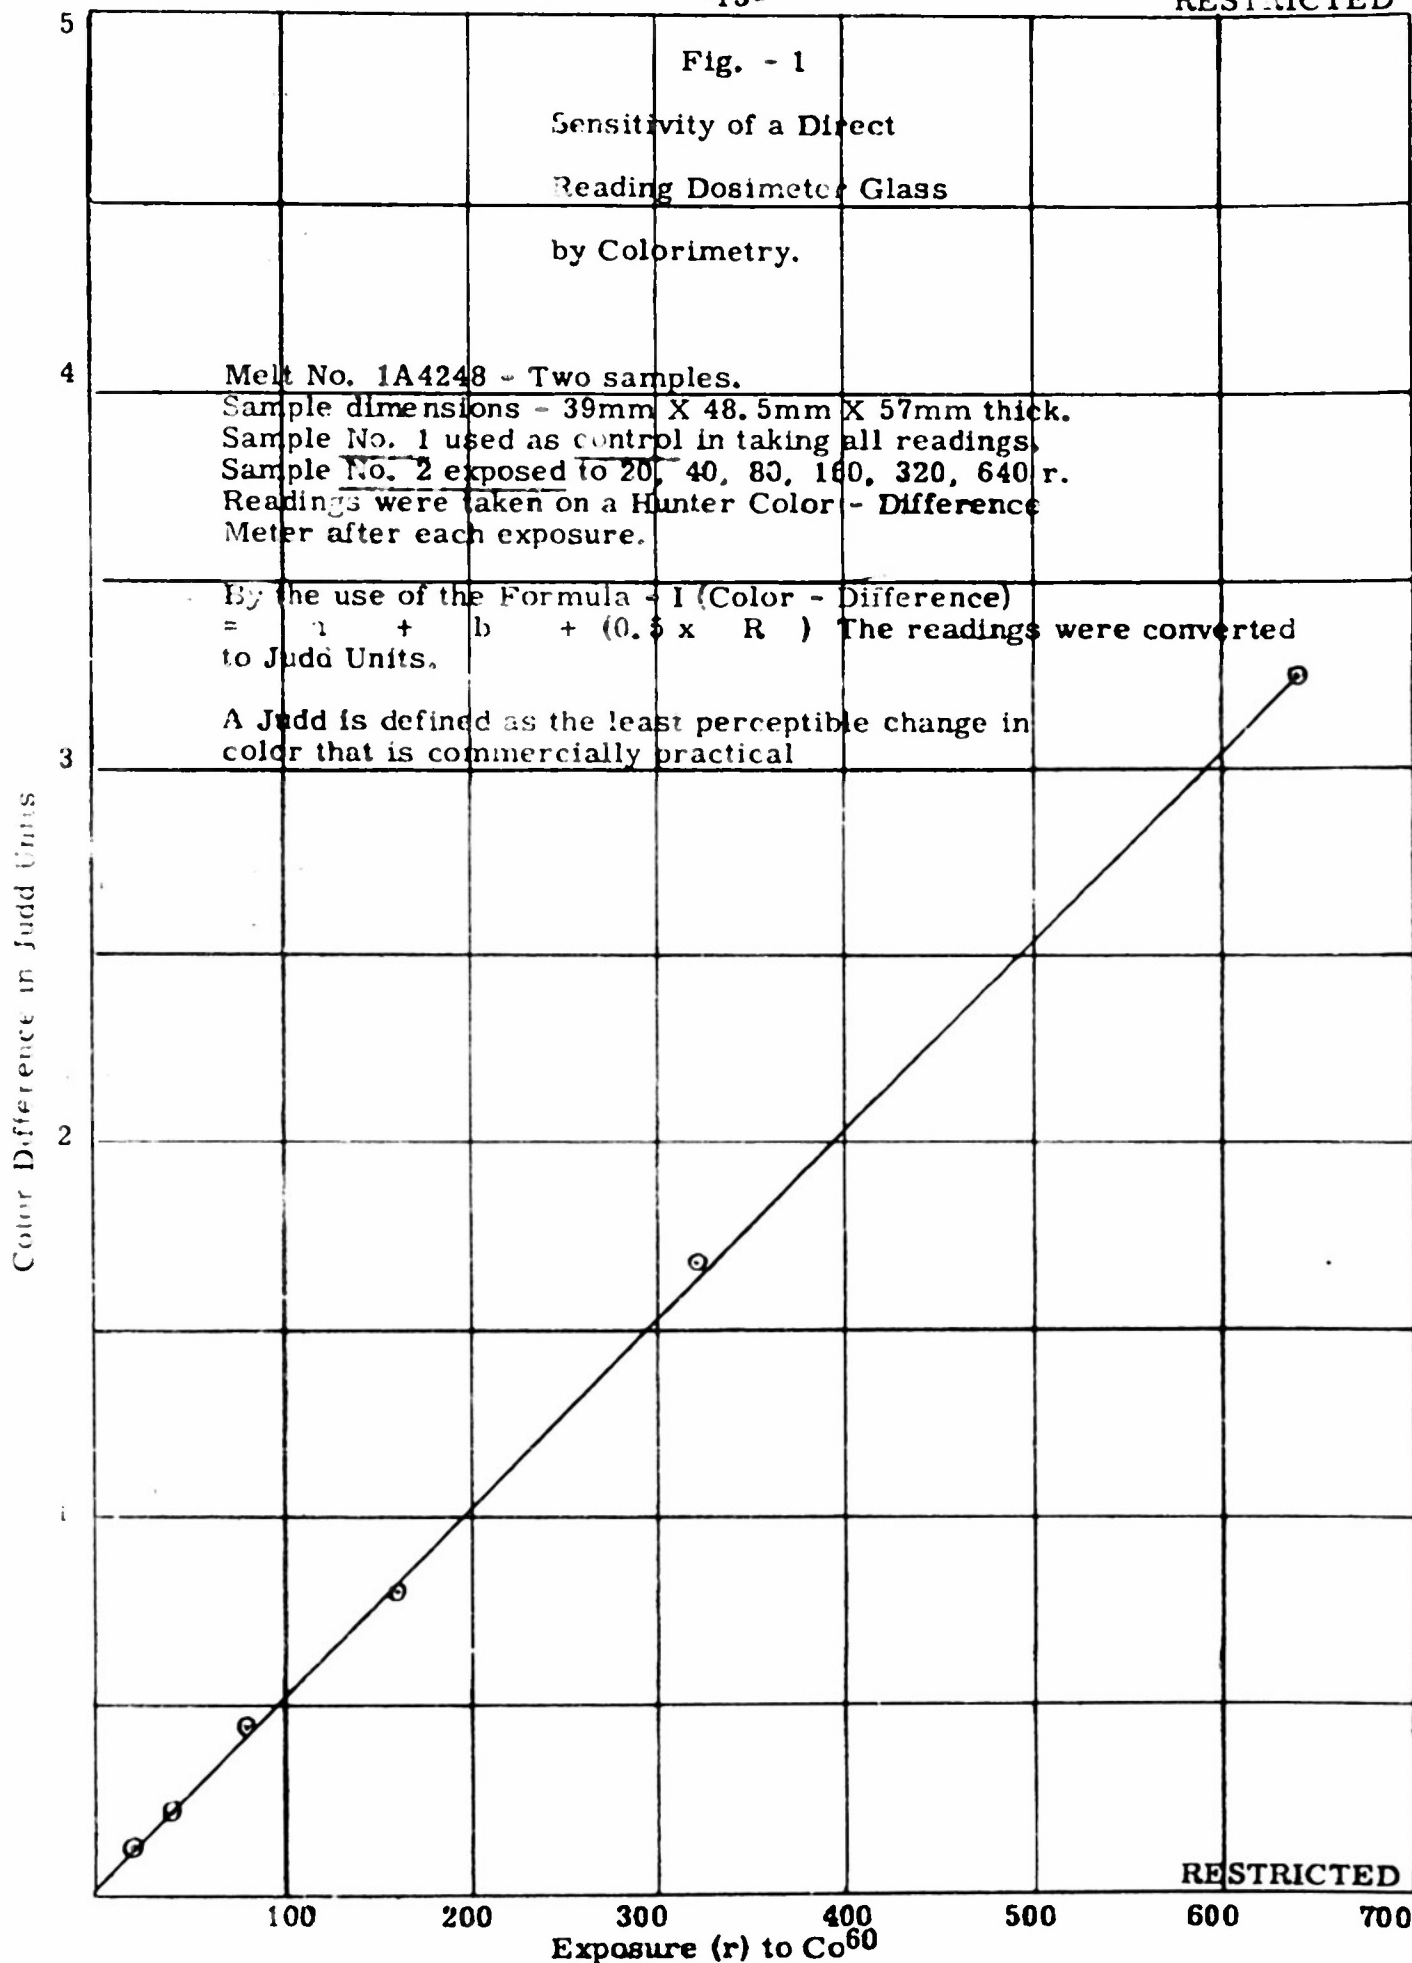


Fig. - 2

Sensitivity of a Direct Reading
Dosimeter Glass by Spectrophotometry

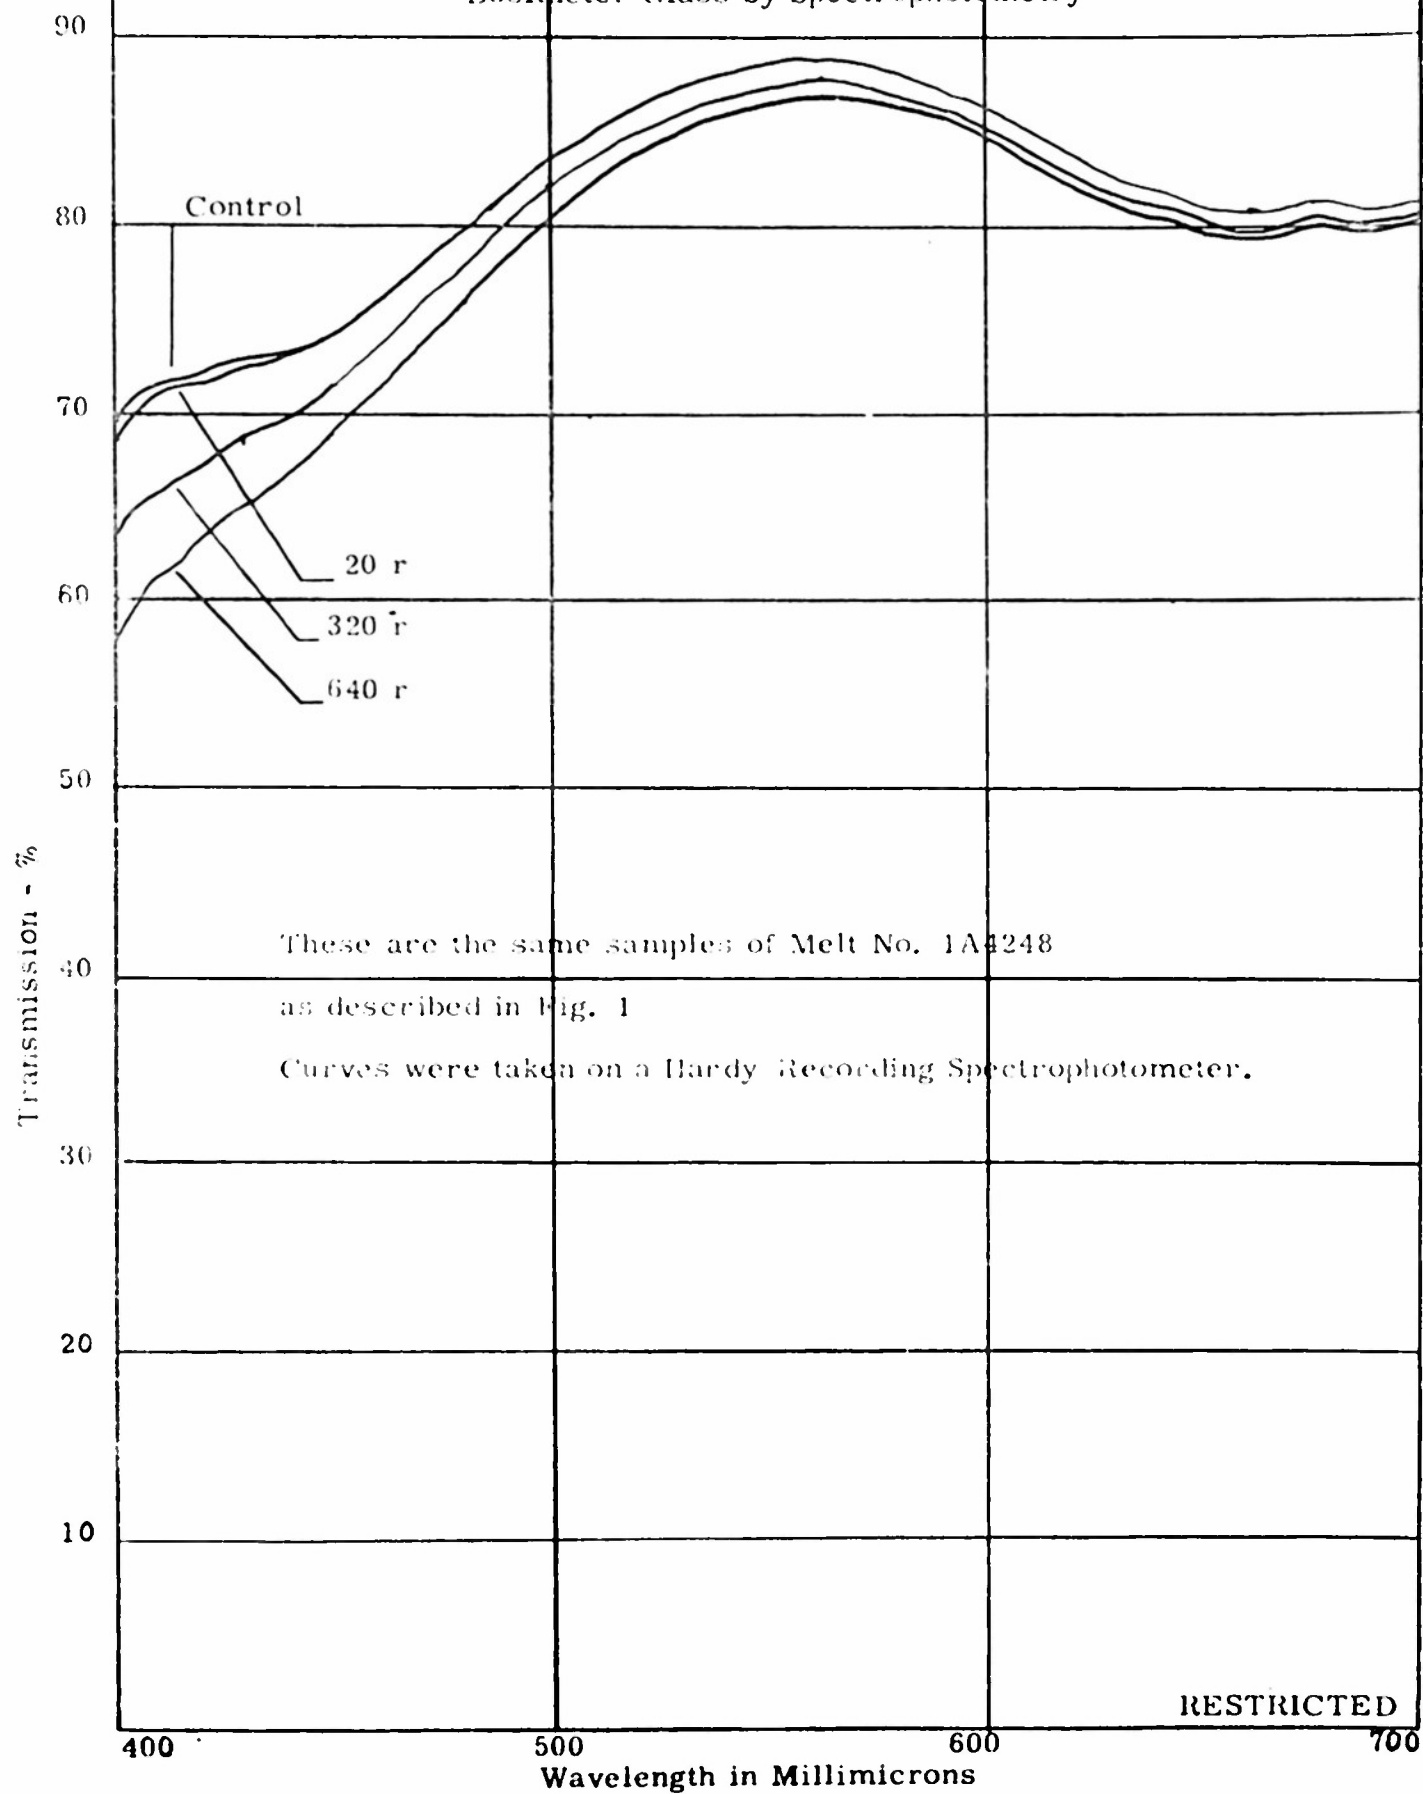


Fig. - 3

Sensitivity of a Direct Reading
Dosimeter Glass by Density
Difference calculated from
Spectrophotometric curves (Fig. 2)

These are the same samples of Melt No.
1A4248 as in Fig. 1

